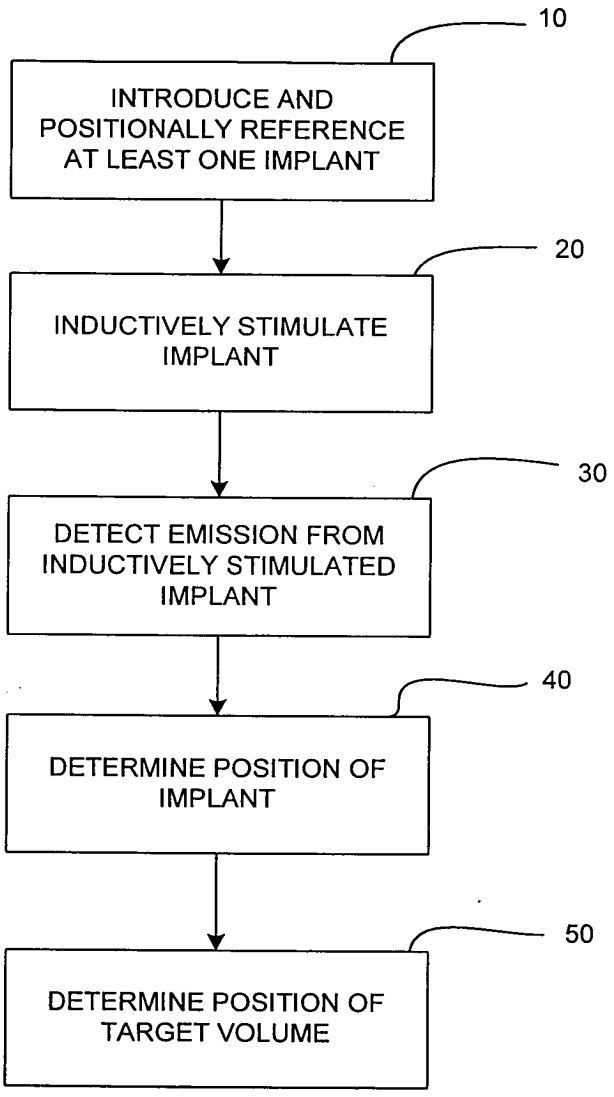
10
INTRODUCE AND POSITIONALLY REFERENCE AT LEAST ONE IMPLANT
20
INDUCTIVELY STIMULATE IMPLANT
30
DETECT EMISSION FROM INDUCTIVELY STIMULATED IMPLANT
40
DETERMINE POSITION OF IMPLANT
50
DETERMINE POSITION OF TARGET VOLUME

FIG. 1